

Quality certificate
 Technical data for Validation
 of LCK529 (0.01-1.0 mg/l
 Copper)

Quality certificate

Technical data for cuvette test LCK529

Sensitivity	0.962 Abs./(mg/l)
Ordinate intersect	0.045 Abs.
Residual standard deviation	0.0097 Abs.
Method variation coefficient	2.08 %
Method standard deviation	0.010 mg/l
Confidence intervall (95%)	± 0.024 mg/l

The technical data for cuvette test LCK529 were determined in conformity with ISO 8466-1 and DIN 38402 A51 „Calibration of analysis methods“.


The series of the smallest and largest calibration standards exhibit normal distribution and are outlier- and trend-free.

The calibration gives a linear function.

Technical data in conformity with DIN 32645

Detection limit	0.0036 mg/l
Quantitation limit	0.011 mg/l

The detection and the quantitation limits were determined in conformity with DIN 32645.

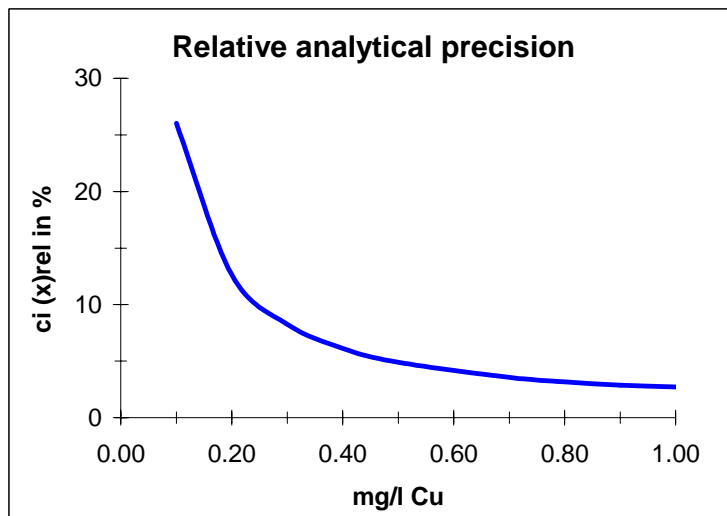

Result	Confidence intervall (95%)
0.2 mg/l	± 0.025 mg/l
0.4 mg/l	± 0.024 mg/l
0.6 mg/l	± 0.024 mg/l
0.8 mg/l	± 0.025 mg/l
1.0 mg/l	± 0.027 mg/l

HACH LANGE GmbH
Quality Management

Dr. Ralf Kloos